



Current 5B 2R 3UV 6V 2022

| | | | |
|-------------------|--------|--------------|-----------------------|
| Cytometer: | LSRII | User: | Administrator |
| Cytometer Name: | LSRII | Institution: | N/A |
| Serial Number: | 1 | Software: | BD FACSDiva 9.0 |
| Input Device: | Manual | Date: | 12/12/2022 4:58:51 PM |
| Window Extension: | 10.00 | | |


Blue Laser
(488nm)
FSC

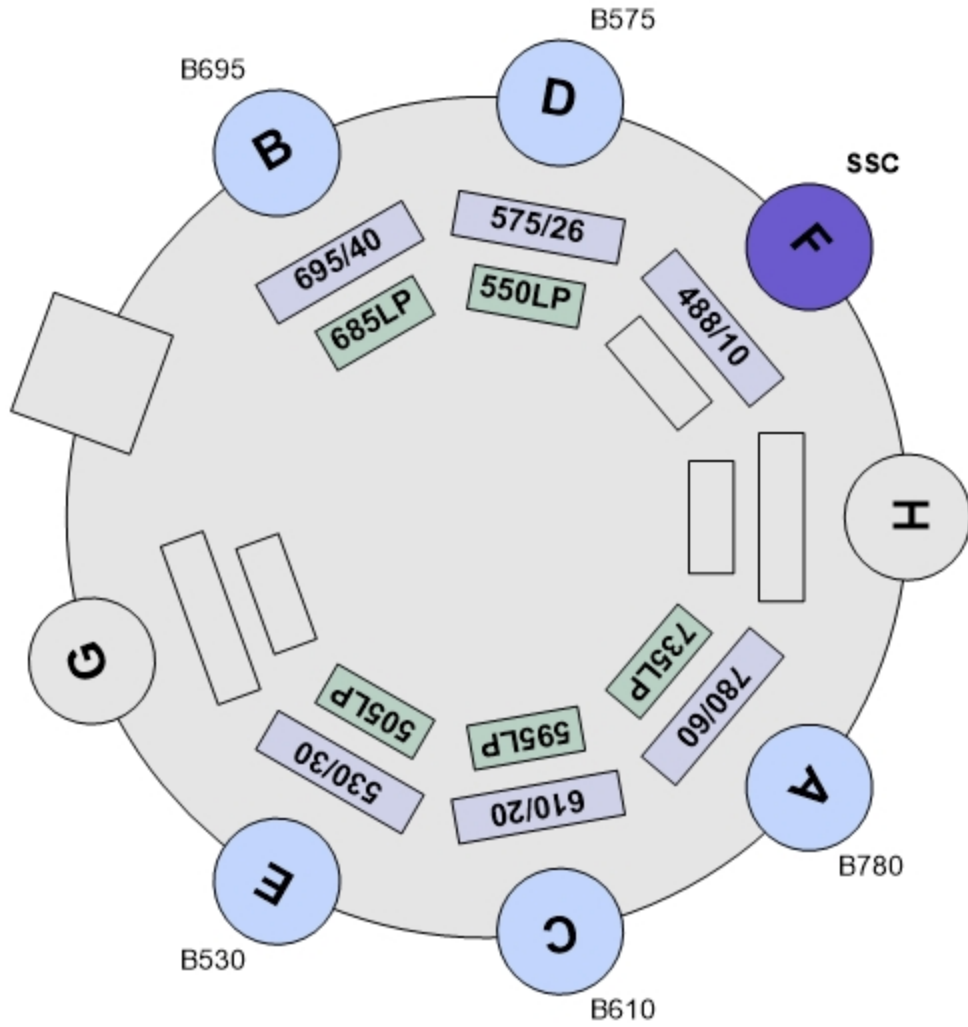


Red Laser
(633nm)

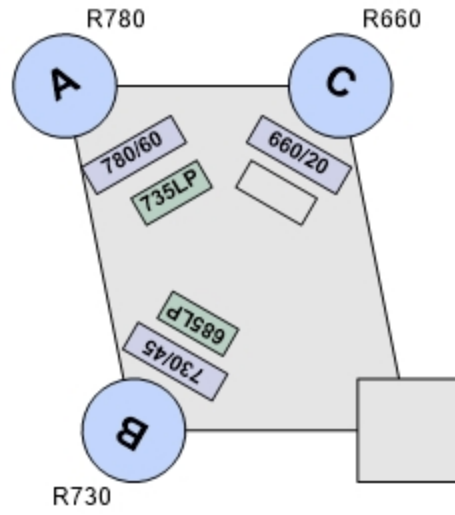

Violet Laser
(407nm)

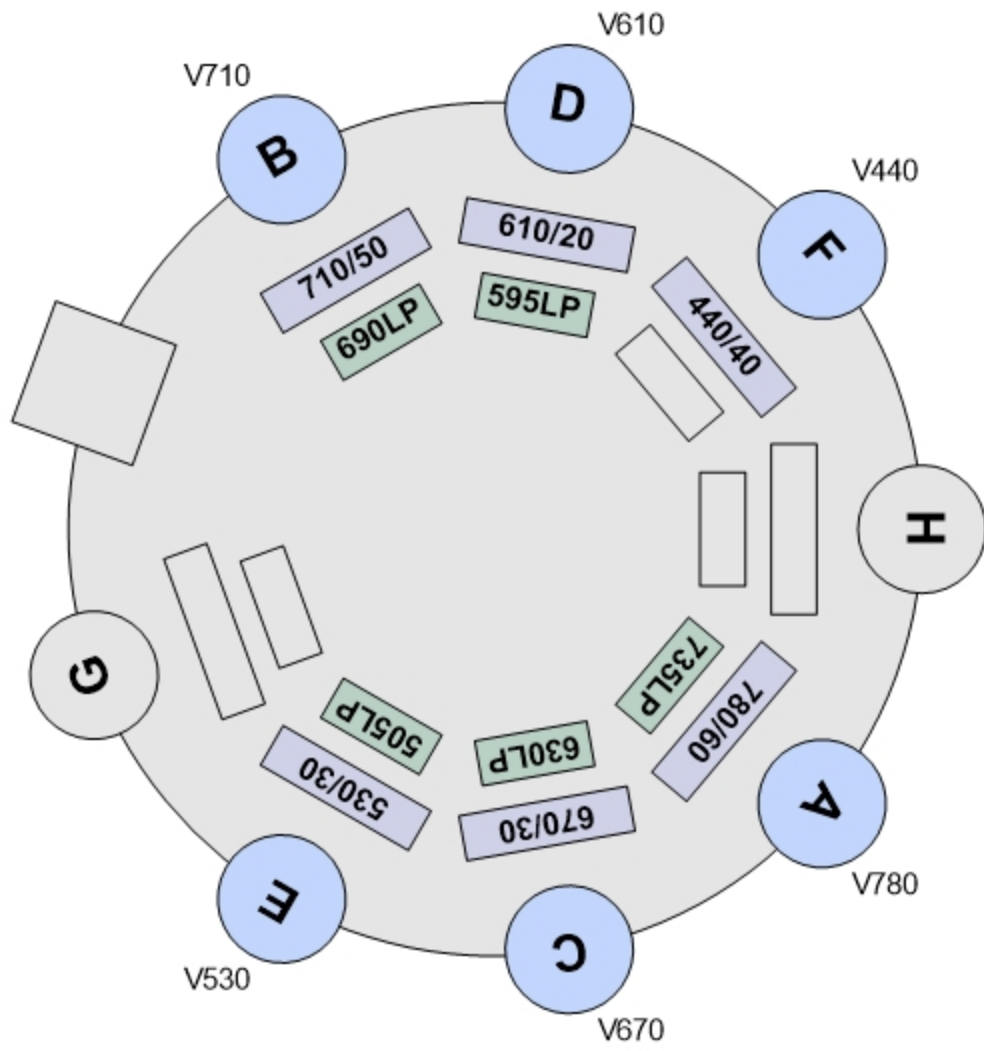

355 UV Laser
(355nm)

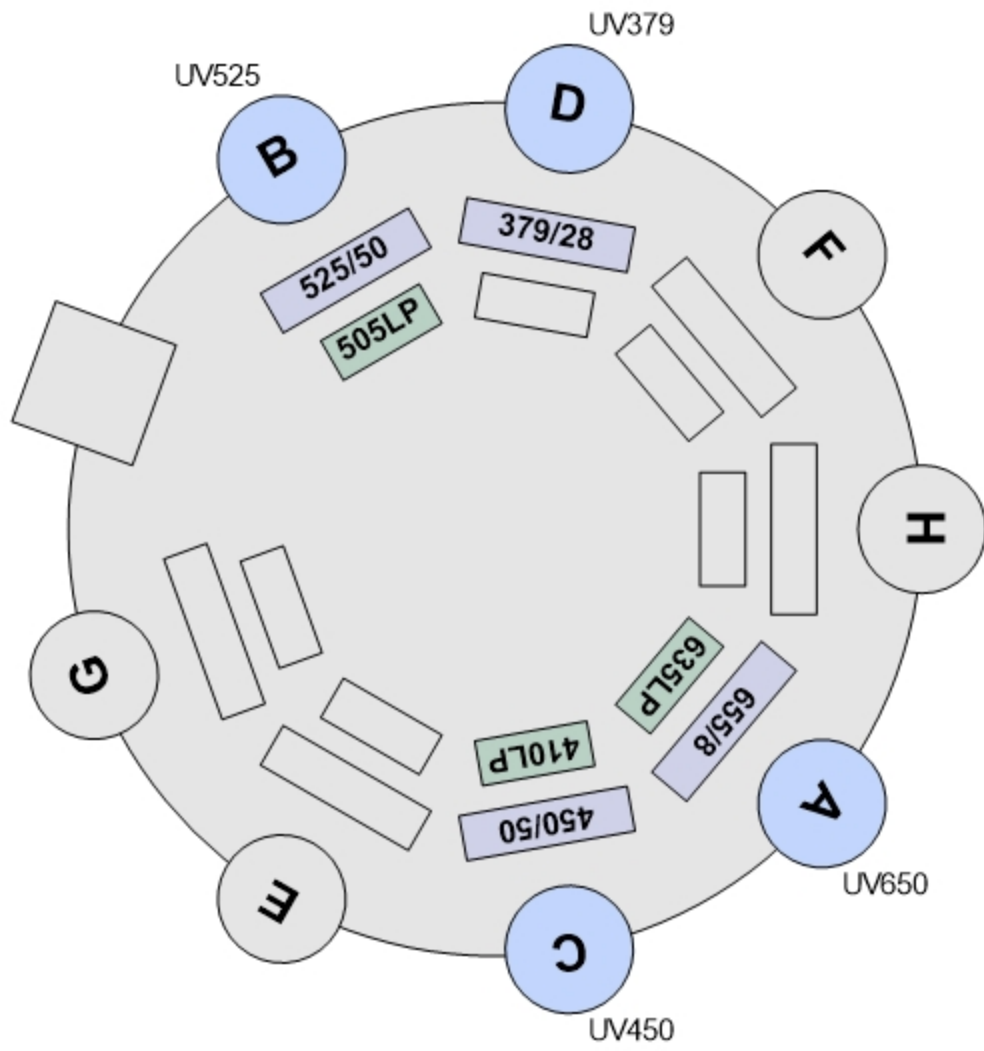

Comments: