



100um20_PSI Universal

Cytometer:	FACSAriaII	User:	Administrator
Cytometer Name:	FACSAriaII	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 9.0.1
Input Device:	Manual	Date:	3/9/2023 8:30:20 AM
Sheath Pressure:	20.00		
Nozzle Size:	100		
Window Extension:	4.00		


Red Laser (640nm)

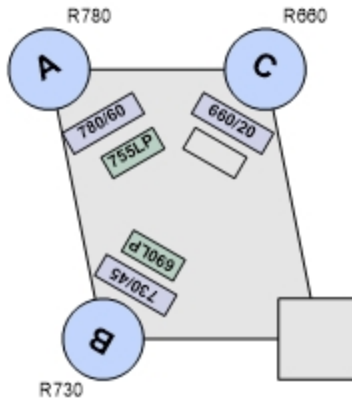


UV Laser (355nm)

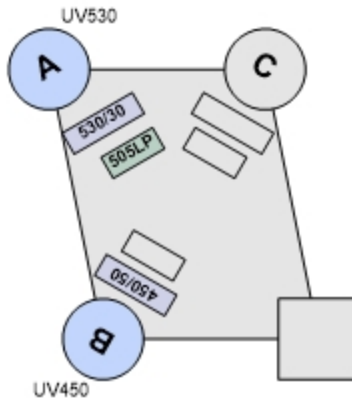


Yellow-Green Laser
(561nm)

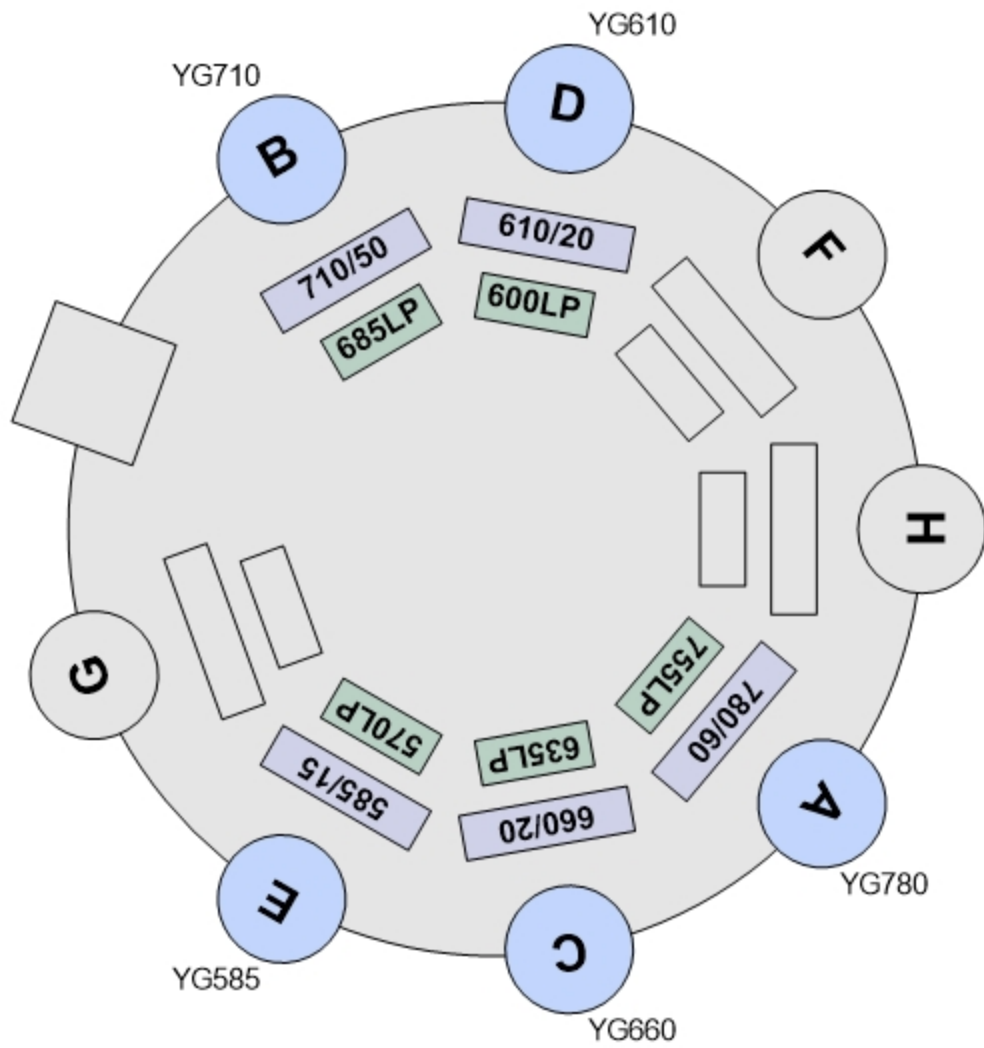

Blue Laser
(488nm)
FSC

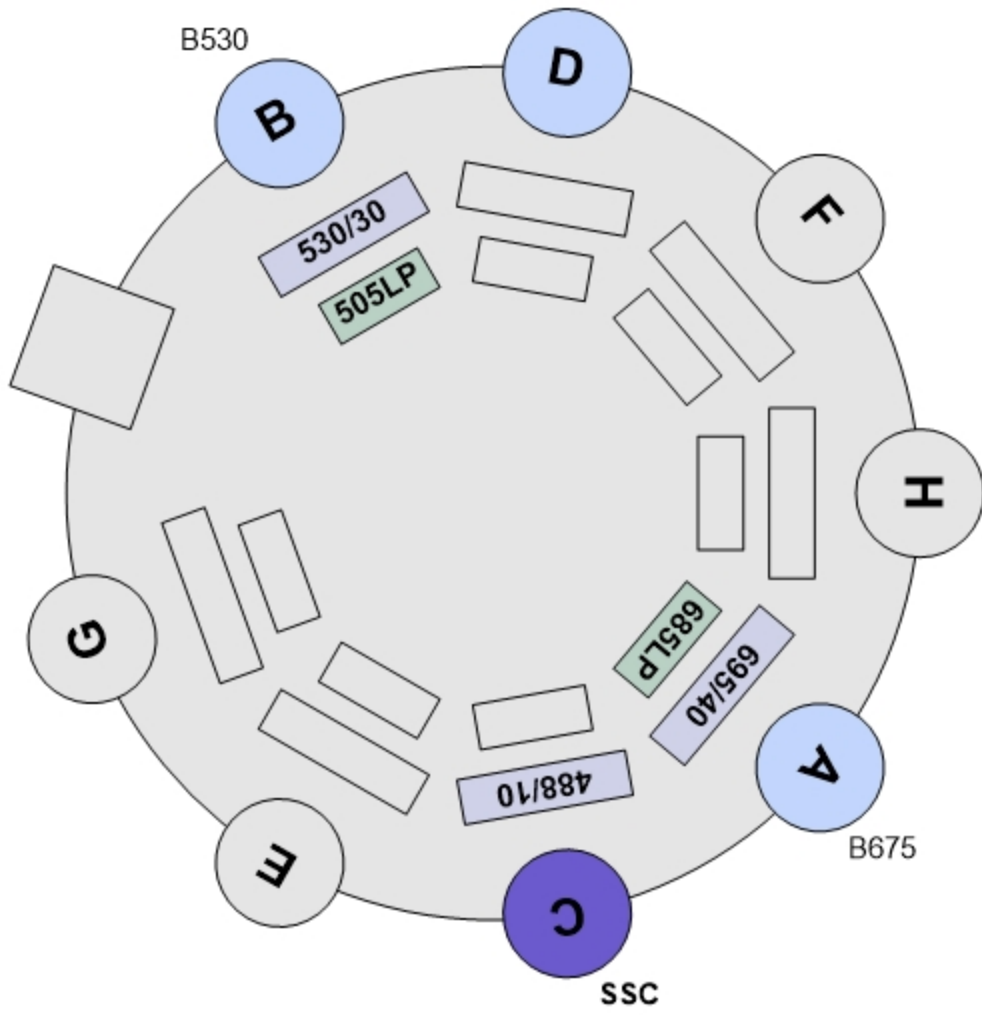

Violet Laser
(405nm)

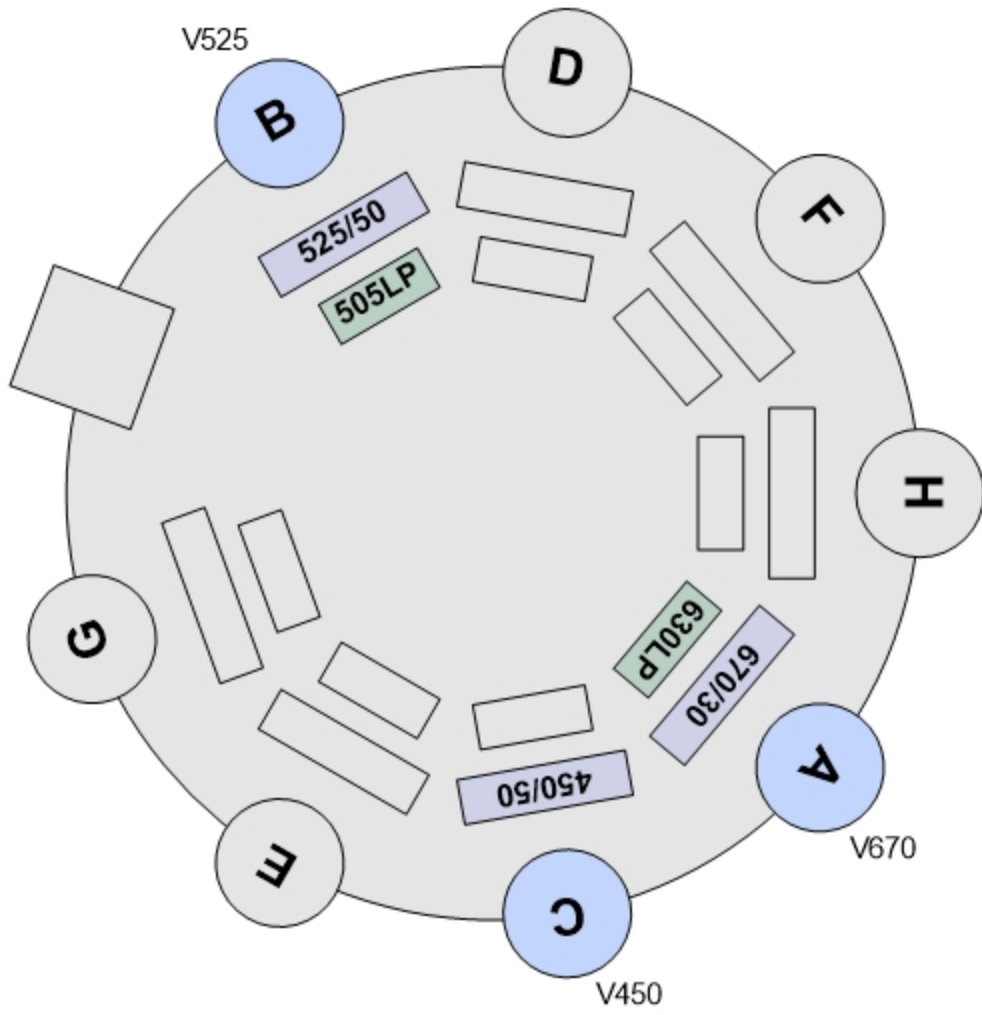

Comments: