



70um70psi Universal

Cytometer:	FACSriaII	User:	Administrator
Cytometer Name:	FACSriaII	Institution:	N/A
Serial Number:	P46900007	Software:	BD FACSDiva 8.0
Input Device:	Manual	Date:	1/21/2020 9:44:55 AM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	4.00		


Red Laser (633nm)

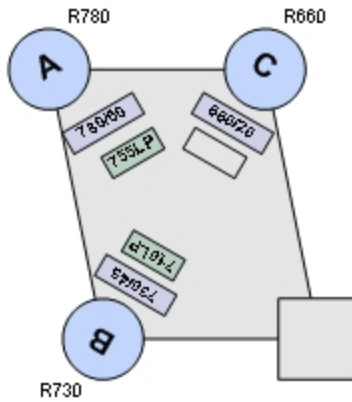


UV Laser (355nm)

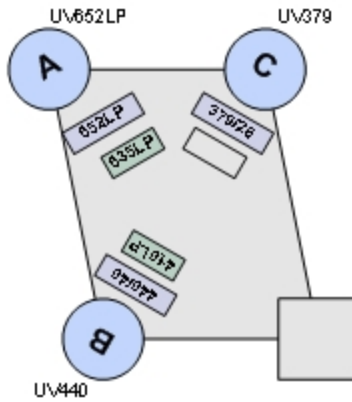


Violet Laser
(407nm)

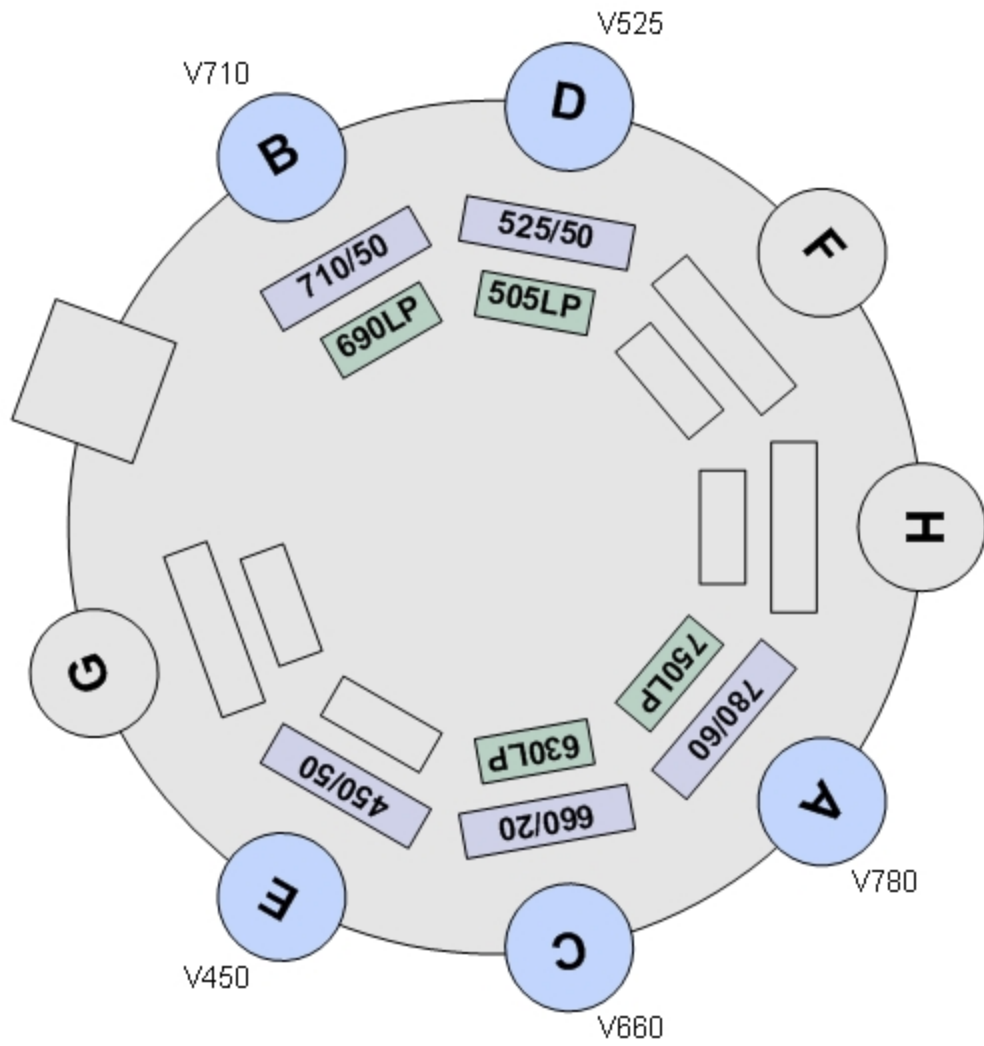

561 Yellow-Green Laser
(561nm)

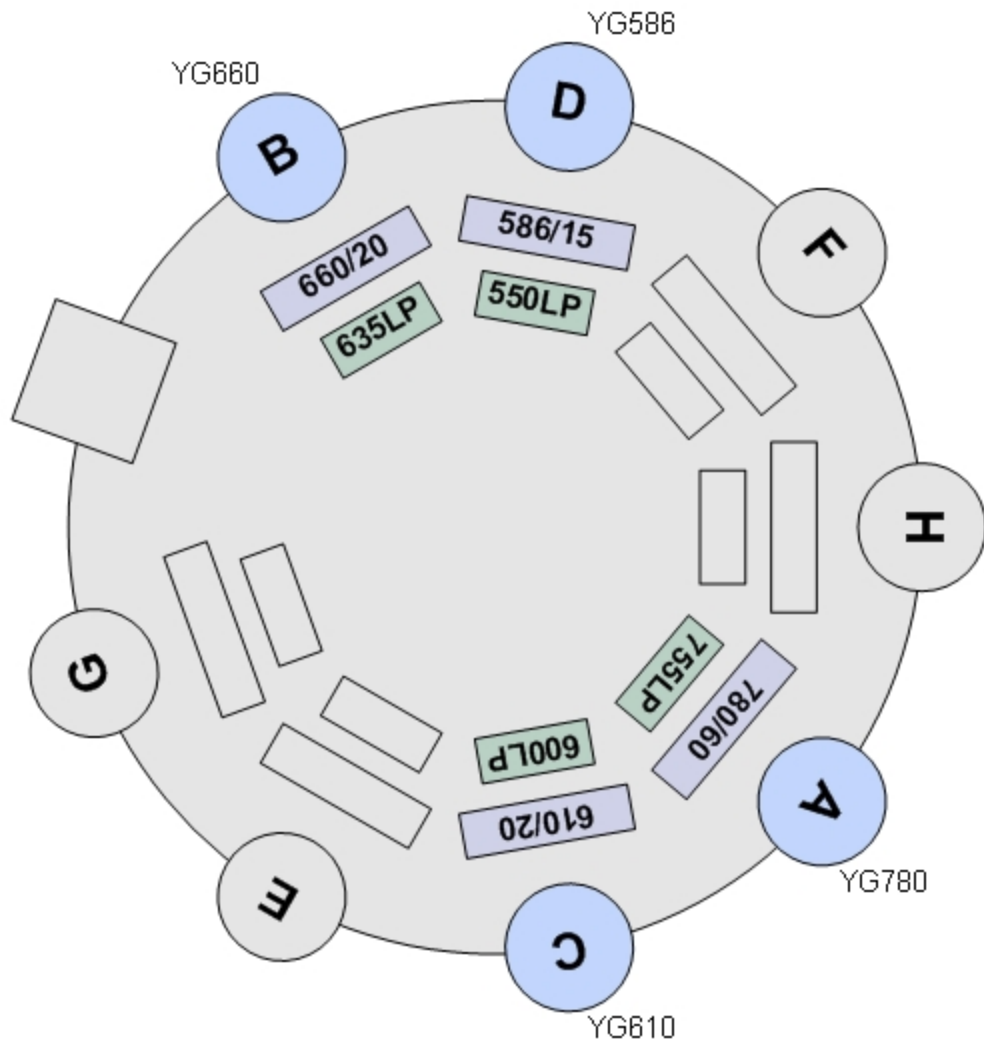

Blue Laser
(488nm)
FSC

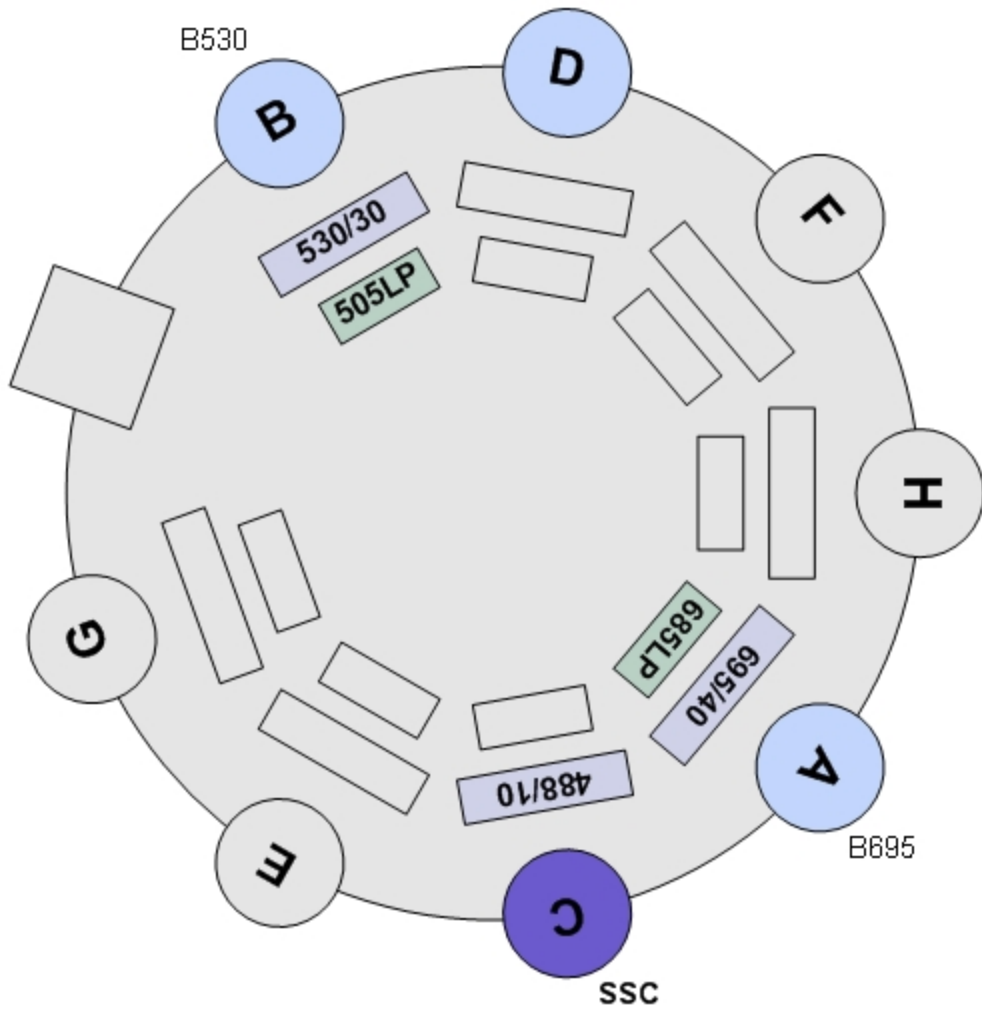

Comments: