



New A5-03092023

| | | | |
|-------------------|--------------|--------------|-----------------------|
| Cytometer: | LSRFortessa | User: | Administrator |
| Cytometer Name: | SymphonyA5 | Institution: | N/A |
| Serial Number: | R66096400091 | Software: | BD FACSDiva 9.3 |
| Input Device: | Manual | Date: | 3/10/2023 10:27:01 AM |
| Window Extension: | 10.00 | | |


Blue Laser
(488nm)
FSC

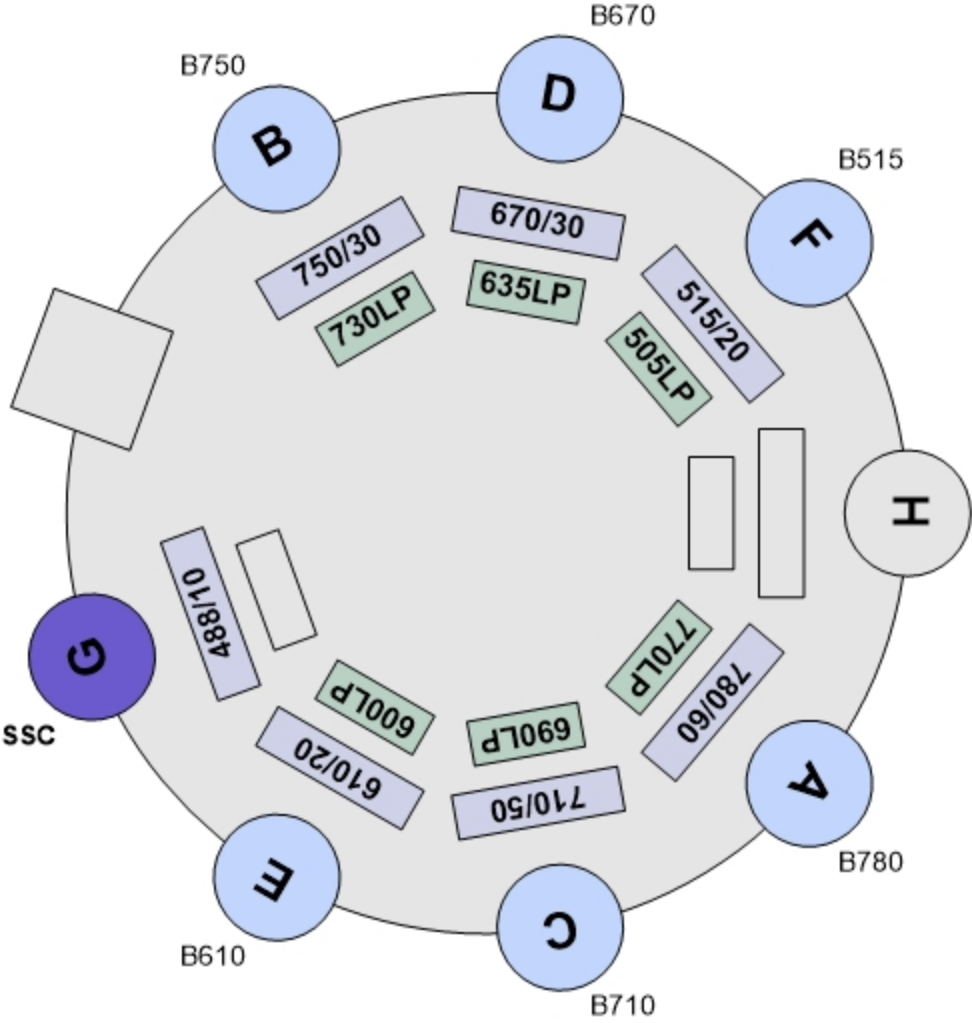


Red Laser
(628nm)

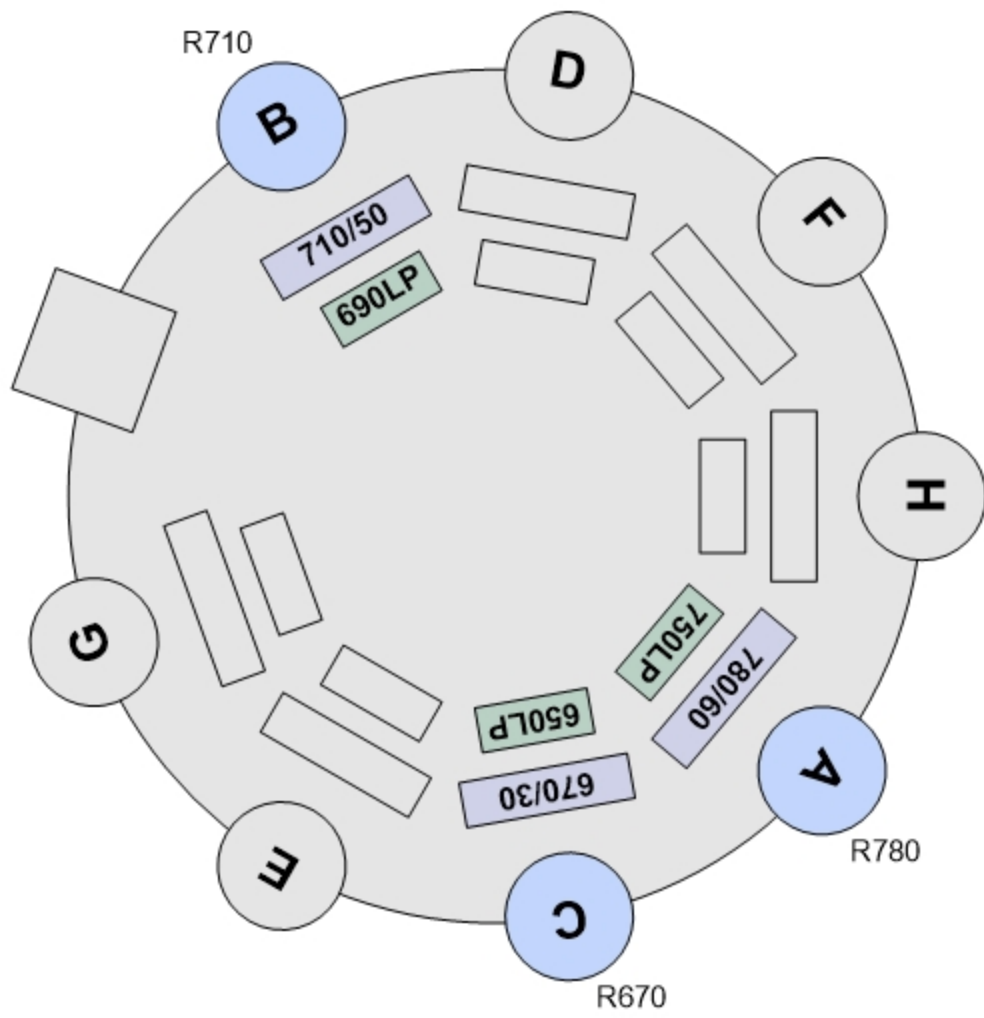

UV Laser
(355nm)

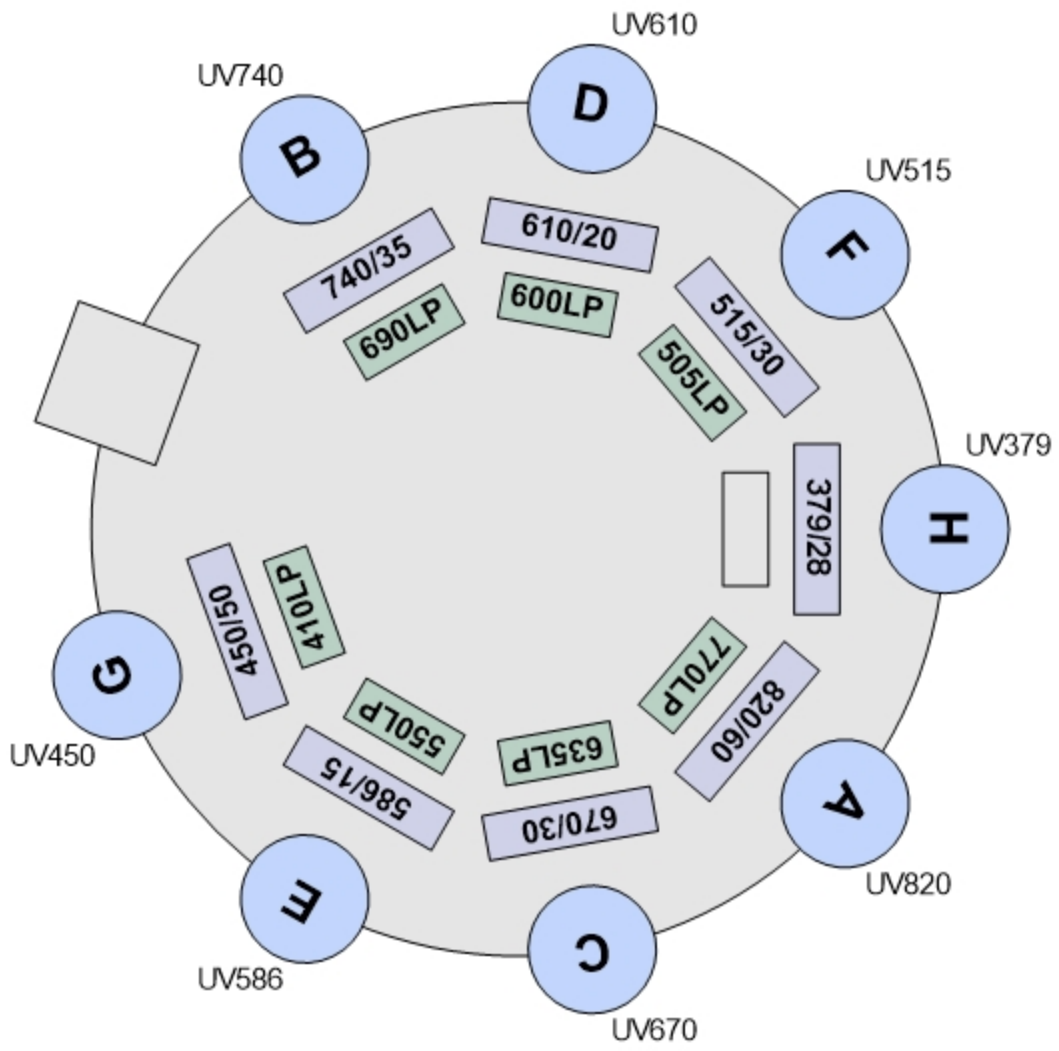

YG Laser
(561nm)

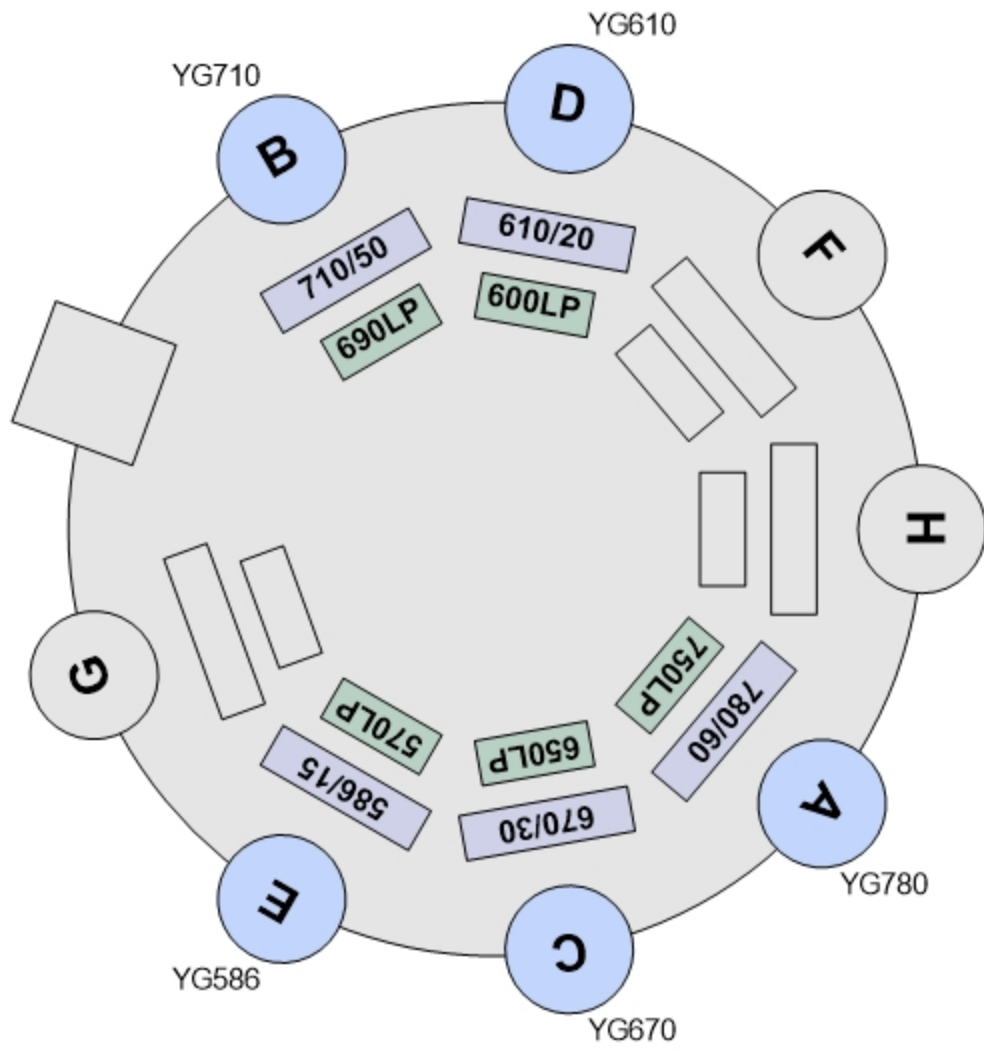

Comments: